

# Rain Gauge Field Verification Kit and Pulse Counter



*Figure 1 - The EML Rainfall Intensity Field Verification Kit with Pulse Counter (P-780-203), The two items, the field verification kit and the pulse counter, are available separately.*

PUBLISHED BY

**Environmental Measurements Limited (EML)**

7 Jupiter Court

Orion Business Park

North Shields NE29 7SE

United Kingdom

Visit our internet pages at <http://www.emltd.net>



©EML 2019

No part of this manual may be reproduced without any form or by any means, electronic or mechanical (including photocopying), nor may its contents be communicated to a third party without prior written permission of the copyright holder.

The contents are subject to change without prior notice.

Please observe that this manual does not create any legally binding obligation for EML towards the customer or end user. All legally binding commitments and agreements are included exclusively in the applicable supply contract or Conditions of Sale.

## Table of Contents

List of Figures .....	3
List of Tables .....	3
<b>1. General Information</b> .....	4
About this Manual.....	4
Version Information .....	4
Related Manuals .....	4
Ordering Information.....	4
<b>2. Product Description</b> .....	5
<b>3. Description of Operation</b> .....	5
<b>4. Maintenance</b> .....	10
<b>5. Statement of Performance in the Laboratory</b> .....	10
<b>6. Specifications</b> .....	11

## List of Figures

Figure 1 - The EML Rainfall Intensity Field Verification Kit with Pulse Counter (P-780-203), The two items, the field verification kit and the pulse counter, are available separately. ....	1
Figure 2 - Three bottles, five brass nozzles, plastic funnel, acetal ring and special acetal bottle-nozzle, comprising the majority of the field verification kit. ....	6
Figure 3: Flow rates and corresponding equivalent rainfall intensities for rain gauges with different orifice areas.....	8
Figure 4 - Flow rates and corresponding equivalent rainfall intensities for rain gauges with different orifice areas (same as Figure 2 but with <b>Log axes</b> ).....	9
Figure 5 - Standardised flow rates for each bottle nozzle combination, with green and red lines showing the +/-5% and +/- 10% limits, respectively. Each boxplot represents nine repetitions (n=9) .....	10

## List of Tables

Table 1 - Document Revisions.....	4
Table 2 - Related Manuals .....	4
Table 3 – Ordering information .....	4
Table 4 - Upper – Showing the ideal tip counts and rainfall depths (mm) for six funnel areas and three bottle sizes, for a 0.2mm per tip rain gauge .....	7
Table 5 - Gauge Specifications for ARG314.....	11

## 1. General Information

### About this Manual

This manual is intended as a general guide for using the Rain Gauge Field Verification Kit and Pulse Counter with different rain gauges. The information contained herein may not cover all aspects of applications. Please refer to associated equipment manuals or consult papers and technical notes on the EML website ([www.emltd.net](http://www.emltd.net)).

### Version Information

*Table 1 - Document Revisions*

<b>EML Document Number:</b>	<b>Description:</b>
Description Rainfall Intensity Field Test Kit_v2.docx	Internal draft version of the User Manual
UM-P-780-203	Version 2.0 - First Release, dated 18/06/2019
UM-P-780-203	Version 2.1 – Minor update, dated 17/07/2019

### Related Manuals

*Table 2 - Related Manuals*

<b>EML Document Number:</b>	<b>Description:</b>
PN3067 - Testing Report May_2019.docx	Testing report carried out on three field verification kits to determine repeatability and produce a combined uncertainty estimate.

### Ordering Information

*Table 3 – Ordering information*

<b>Product code</b>	<b>Description</b>
P-780-202	Digital Pulse Counter
P-780-203	Rain Gauge Field Verification Kit with Pulse Counter
P-780-204	Rain Gauge Field Verification Kit (No Pulse Counter)

## 2. Product Description

The EML field verification kit is a simple mechanical device which can be used to simulate five different flow rates. By using three sizes of bottle, the approximate duration of each testing schedule can be planned based on a field engineer's available time. Figure 1 on the first page of this manual shows a picture of the field verification kit (P-780-204) and the pulse counter (P-780-202). The kit can be purchased with or without the pulse counter, which is the square box on the right-hand side of Figure 1. See the Ordering Information on Page 5 for more details. If the pulse counter is included, the full kit is comprised of:

- a) Three bottles of different sizes (**147ml, 298ml and 530ml** – when filled to the brim)
- b) A funnel with five nozzle attachments, each with a different hole diameter (**0.6, 1.0, 1.2, 1.5 and 2.0mm**)
- c) Bubbler device and acetal covering to ensure a constant head during tests
- d) Aluminium lined carrying case (shown in Figure 1)
- e) A clear Perspex plate to put across the rain gauge orifice (suitable for orifices up to 500cm<sup>2</sup>) – shown at the back of the case in Figure 1
- f) Pulse counter and cable to record the number of tips – shown as the box on the right hand side of Figure 1 (for tipping bucket gauges or weighing rain gauges with a tipping bucket output)

## 3. Description of Operation

- 1) Connect the counter to the rain gauge, if using a tipping bucket rain gauge (TBR) or connect the gauge to a PC or other suitable device, if using a weighing gauge or digital-output TBR.
- 2) Ensure the gauge is level and place the Perspex plate on top of the gauge orifice.
- 3) An appropriate brass nozzle and bottle combination is selected from Table 4 (lower left) and described on page 6.
- 4) Fill the bottle **to the brim** with water and screw the special plastic nozzle cap onto the cutaway bottle cap - shown on top of the medium bottle in the middle of Figure 2.
- 5) The appropriate brass nozzle is placed on the end of the funnel, like in Figure 2.
- 6) Place the acetal plastic piece inside the top of the funnel and position so that the brass nozzle is pointing upwards (as shown in Figure 2). Then, place this over the top of the selected bottle.  
**NB:** in order to prolong the lifespan of the plastic funnel, do not force the brass nozzle on.
- 7) Take these pieces in hand, and tip them into the hole in the Perspex plate which is sitting on top of the rain gauge. They should fit snugly, allowing no rainfall to get into the rain gauge if it is raining while the tests are being performed. **To watch a video of this process, [click here.](#)**
- 8) It is good practice to make a note of the time the test starts.
- 9) Once the water has totally drained from the bottle and the test is completed, note the value shown on the counter or PC.
- 10) Repeat this procedure for the required number of tests/intensities using different bottle and nozzle combinations.



Figure 2 - Three bottles, five brass nozzles, plastic funnel, acetal ring and special acetal bottle-nozzle, comprising the majority of the field verification kit.

Table 4 (upper) shows the ideal expected tip counts (**red**) and the equivalent rainfall depths (**green**) for a range of different rain gauge funnel areas, for each of the three bottle sizes. Note that if partial tips are not taken into account, then it is important to **round down** these values. An example is provided in the line of text underneath this sub-table, marked with an asterisk (\*).

Table 4 (lower left-hand side) shows test durations for different combinations of bottle size and nozzle diameter. This should be used to plan the testing schedule. Only the recommended operationally practical tests have been included in this table (**green**), whereas less practical combinations of bottle and nozzle have been marked with a red **X**. The recommended minimum test time is 3 minutes for the largest nozzle, in order to try to limit any edge effects at the beginning and end of the tests, such as partial filling of the tipping bucket mechanism. In general, a longer test will provide a more reliable flow rate. This part of the table also displays the average flow rate generated by each nozzle.

The lower right-hand side of Table 4 (on the right of the blue arrows) shows columns of the equivalent rainfall intensity in mm/hr for five rain gauges, with orifice areas marked in cm<sup>2</sup>.

Figure 3 and Figure 4 are plots showing the correspondence between flow rate and equivalent rainfall intensity for rain gauges with different orifice areas. They are included for reference. Figure 3 uses standard axes and Figure 4 uses Log axes, which makes the lower intensities easier to read.

Table 4 - Upper – Showing the ideal tip counts and rainfall depths (mm) for six funnel areas and three bottle sizes, for a 0.2mm per tip rain gauge

**Lower left-hand side of dotted line:** Showing the test durations of different combinations nozzle diameter and bottle size. Also shows the average flow rate for each nozzle diameter.

**Lower right-hand side of dotted line:** Showing the equivalent rainfall intensities corresponding to each flow rate for rain gauges with different orifice areas, in cm<sup>2</sup>

Bottle Size (ml)	Ideal *tip count* / *rainfall depth* for 0.2mm per tip gauges with funnel collecting areas of:					
	127cm <sup>2</sup>	200cm <sup>2</sup>	314cm <sup>2</sup>	324cm <sup>2</sup>	400cm <sup>2</sup>	500cm <sup>2</sup>
Small (147)	58.1 / 11.62 mm	36.8 / 7.35 mm	23.4 / 4.68 mm	22.7 / 4.54 mm	18.4 / 3.68 mm	14.7 / 2.94mm*
Medium (298)	117.8 / 23.56 mm	74.5 / 14.90 mm	47.5 / 9.49 mm	46.0 / 9.20 mm	37.3 / 7.45 mm	29.8 / 5.96 mm
Large (530)	209.5 / 41.9 mm	132.5 / 26.50 mm	84.4 / 16.88 mm	81.8 / 16.36 mm	66.3 / 13.25 mm	53.0 / 10.6 mm

\*Important Note: when not measuring partial tips, all values should be **rounded down** appropriately, either to the nearest full tip, or to the nearest 0.2mm increment e.g. grey highlighted cell would read: **14.0 / 2.8mm**

		Bottle Size (Volume in ml):			Flow Rate (m/min) [Approx. Ave.]:	Equivalent Rainfall Intensity (mm/hr) for Gauge Area cm <sup>2</sup> :					
		S (147)	M (298)	L (530)		127(Kalyx)	200(Pluvio)	314(SBS314)	324(EA)	400(Casella)	500(SBS500)
Nozzle diameter (mm):	0.6	12.9	X	X	11	52	33	21	20	16	13
	1.0	X	8.8	X	34	161	102	65	63	51	41
	1.2	X	5.8	X	52	246	156	100	96	78	41
	1.5	X	X	5.4	98	464	294	187	182	147	118
	2.0	X	X	3.2	166	786	498	317	308	249	199
		Av. time to empty (mins):									

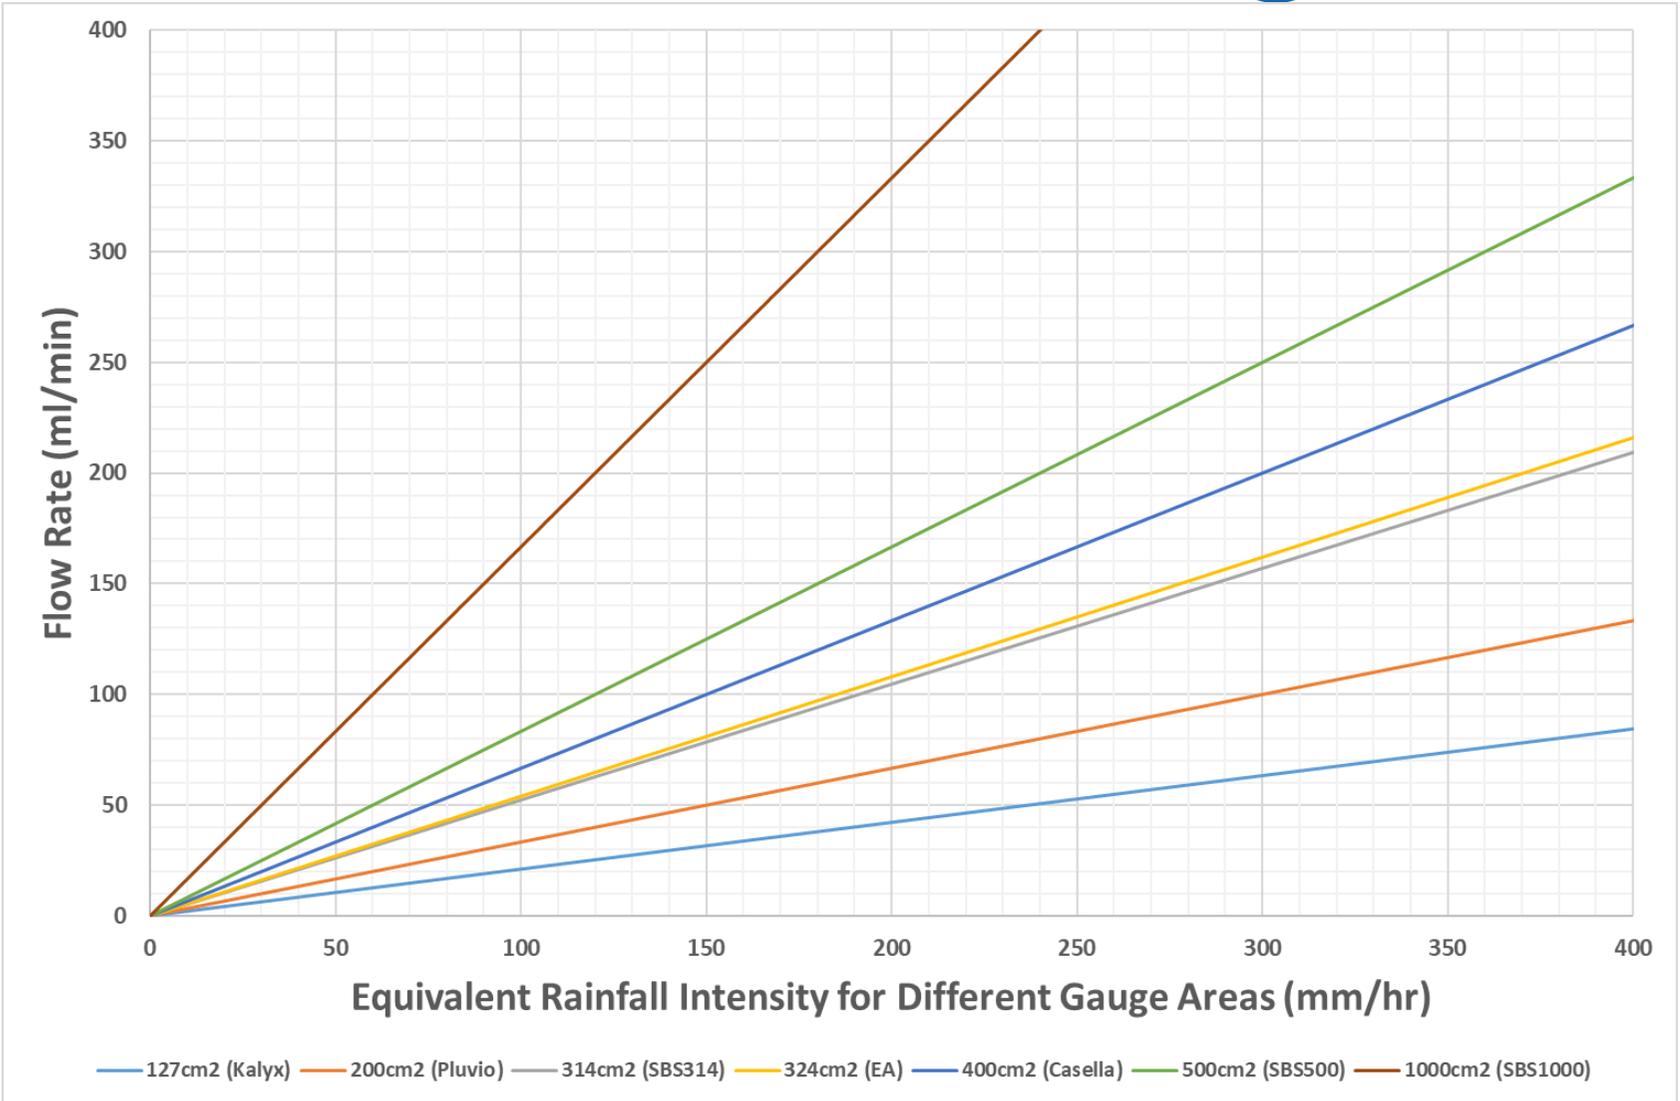


Figure 3 - Flow rates and corresponding equivalent rainfall intensities for rain gauges with different orifice areas

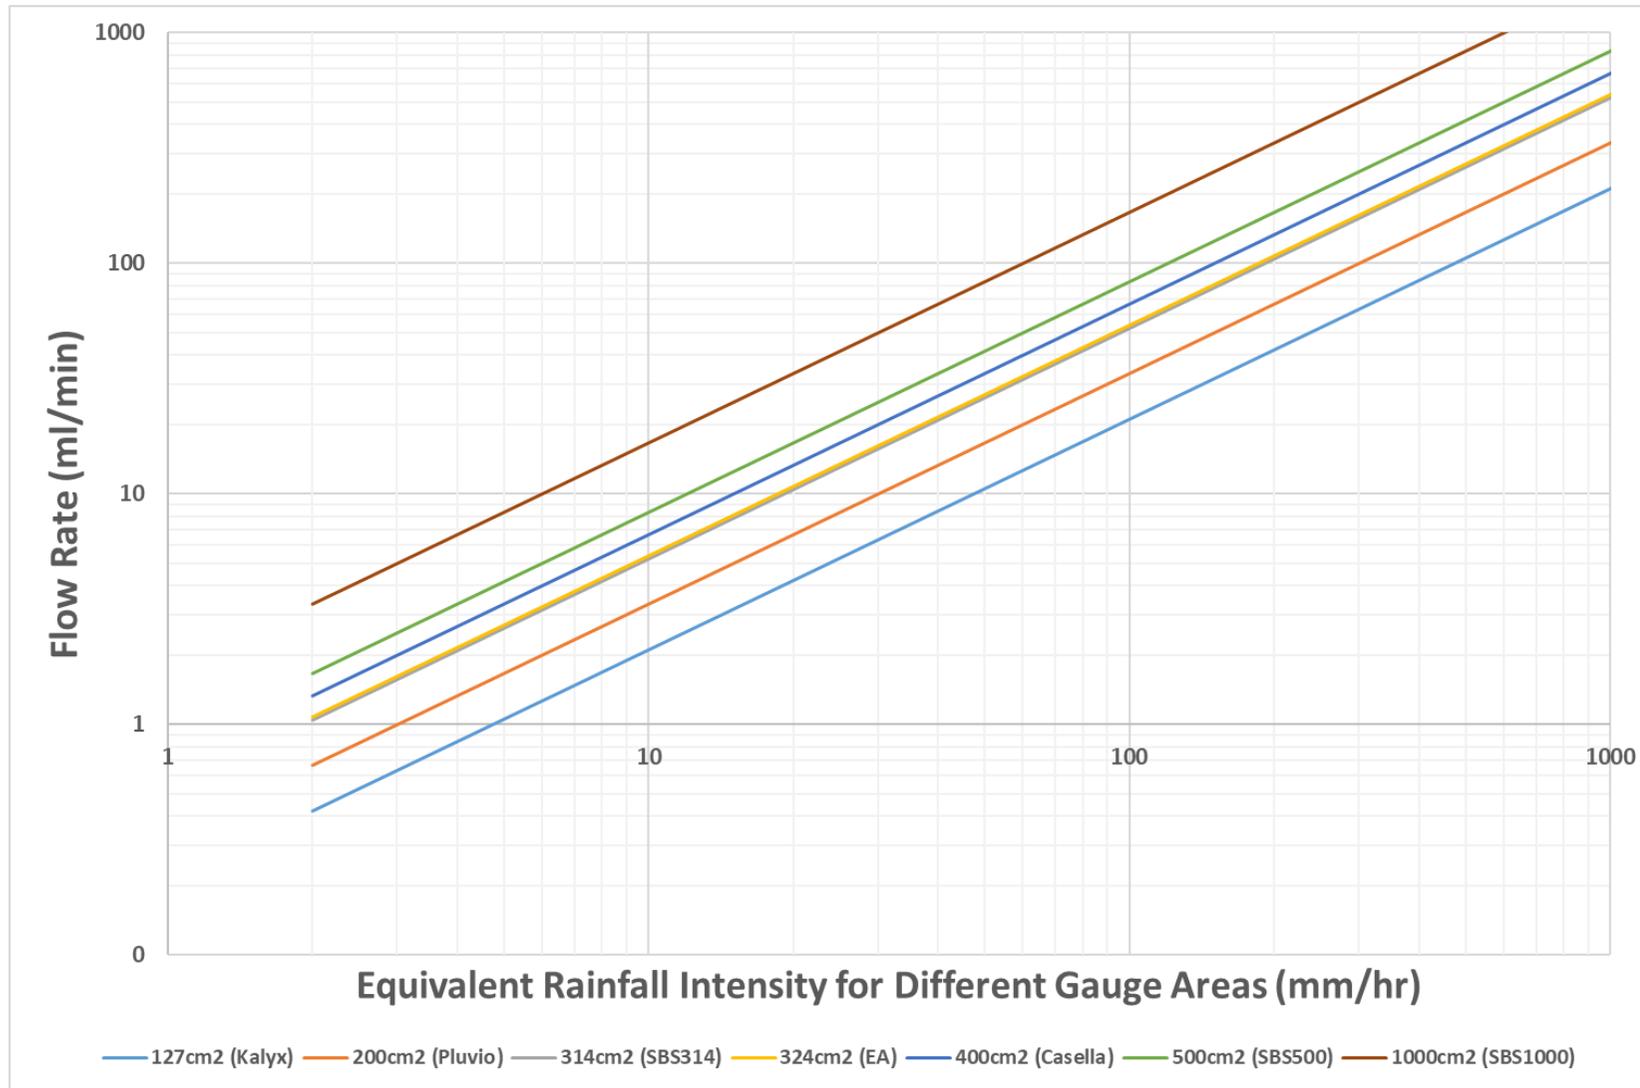


Figure 4 - Flow rates and corresponding equivalent rainfall intensities for rain gauges with different orifice areas (same as Figure 2 but with **Log axes**)

## 4. Maintenance

To ensure good repeatability of the brass nozzles, it is important to keep them free from dust and dirt. This is particularly important for the nozzles with the smallest diameter holes, i.e. the 0.6mm and the 1.0mm, which tend to become blocked or partially blocked more easily, thus affecting the flow rate. To clear dirt and dust from the holes, a total of five drill-bits have been included, one for each nozzle. **NOTE:** Care must be taken not to force a larger drill-bit into a hole which is smaller than the drill-bit itself, otherwise the hole will be damaged, and the flow rates will alter.

## 5. Statement of Performance in the Laboratory

To test the performance of the field verification kits, a full testing schedule was developed, and a report produced. That report is available on request. To summarise the results of the report, the testing schedule was performed on three field verification kits, with an assessment of the combined uncertainty value produced for each of the five nozzles. The applicability of this user manual hinges on the repeatability of performance between multiple field test kits. More information can be found in the test report, but after a total of 45 repetitions on three field test kits, the results indicated that 87% of the test data were within +/- 5% of the mean value, and 100% was within +/-10%. This is summarised in the following plot, where each boxplot represents one bottle-nozzle combination (shown on the x-axis), and where the y-axis shows the flow rates standardised by the appropriate average flow rate. A summary of the achievable accuracy is supplied in the Table 5 in Section 6 (page 11).

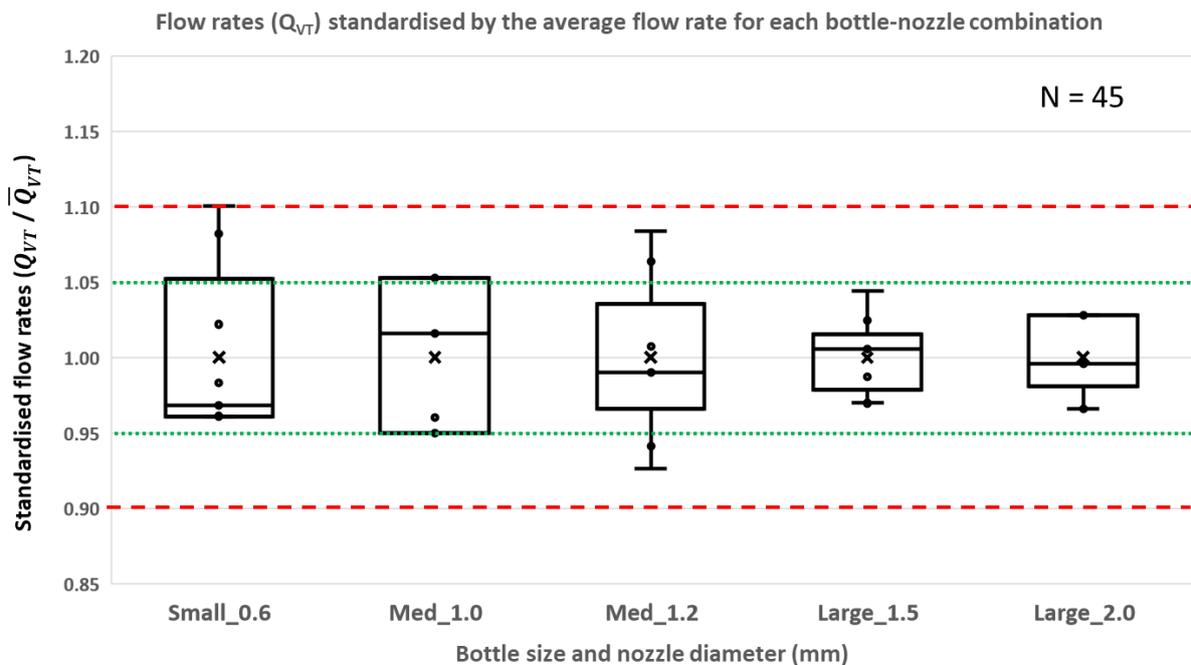


Figure 5 - Standardised flow rates for each bottle nozzle combination, with green and red lines showing the +/-5% and +/-10% limits, respectively. Each boxplot represents nine repetitions (n=9)

## 6. Specifications

Table 5 - Gauge Specifications for ARG314

Technical Specifications			
Precision / Repeatability	<b>Nozzle Diameter</b>	<b>Flow Rate</b>	<b>Repeatability</b>
	0.6mm	11 ml/min	+/- 10%
	1.0mm	34 ml/min	+/- 10%
	1.2mm	52 ml/min	+/-10%
	1.5mm	98 ml/min	+/- 5%
	2.0mm	166 ml/min	+/- 5%
Rainfall Intensity	Rainfall intensity depends on gauge orifice area. See Table 4 for conversion information.		
Rain Gauge Collecting Areas	127cm <sup>2</sup> – 500cm <sup>2</sup>		
Operating Temperature	0°C - 60°C		
Weight	3Kg		